




KONICA MINOLTA

Traceability System for Chroma Meter CR-300 & CR-400 Series

January, 2004

Konica Minolta Photo Imaging Europe GmbH
Instrument Systems Division

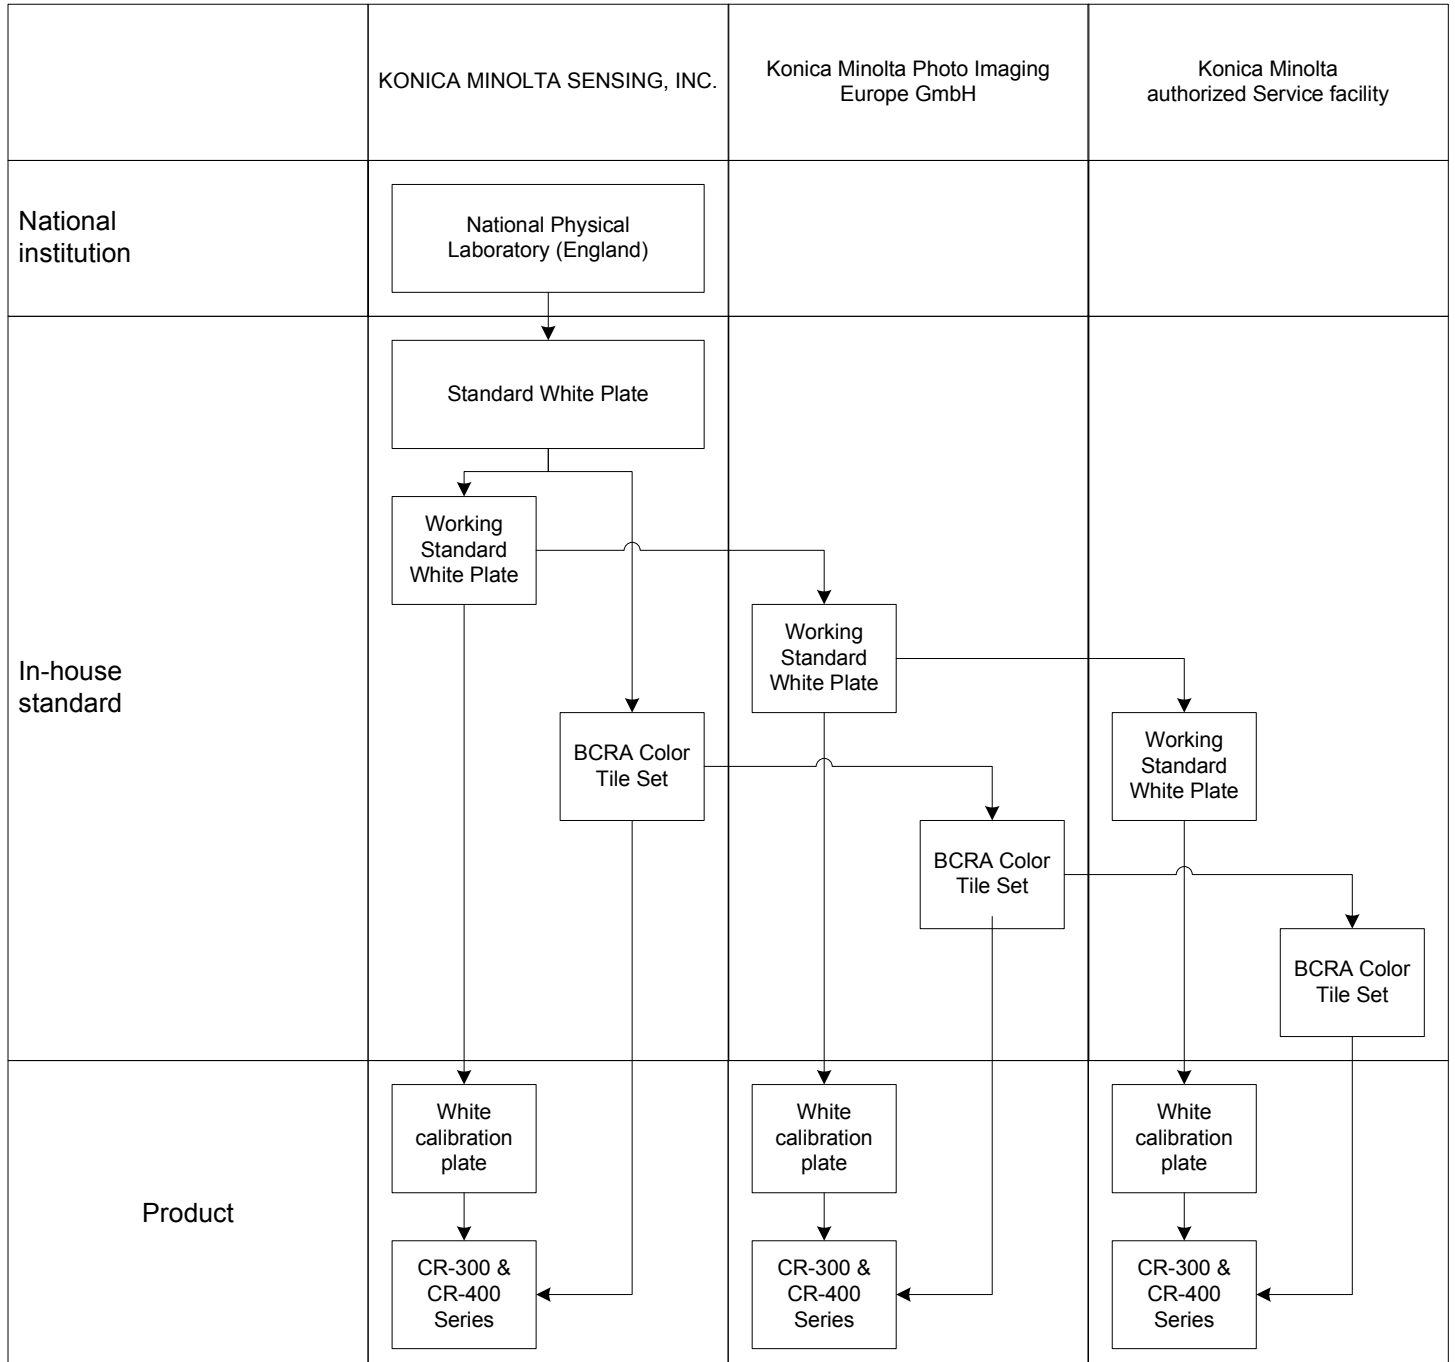

Interval between calibration:

Standard White Plate: 5 years

Working Standard White Plate: 1 year

BCRA Color Tile Set: 1 year